

IVD CE



Certificated site: Kamishima Factory, Sales Department

hMPV Ag

Capilia™ hMPV



* The sample shows positive result.

Rapid test for Human Metapneumovirus (hMPV) antigens

Permitting accurate results; simple and easy to use

Easy to read Black Line

Adopting the latest nanotechnology, "Platinum-Gold Colloid"

Fast test results


Reading time is 3-5 min.

Shared use of extraction buffer in Capilia series


1 sample can be used for 4 types of tests (Flu, Adeno, RSV, hMPV)




more reasonable process, less pain for patients



Collecting specimen



Preparing sample

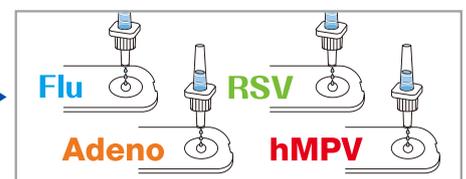

1 sample can be used for up to 4 test plates!

Please follow package insert with each product about shared use of extraction buffer.


Capilia™ hMPV




To detect Human Metapneumovirus antigens in nasal swab, nasal aspirate or pharyngeal swab.

Test procedure

Method of specimen collection


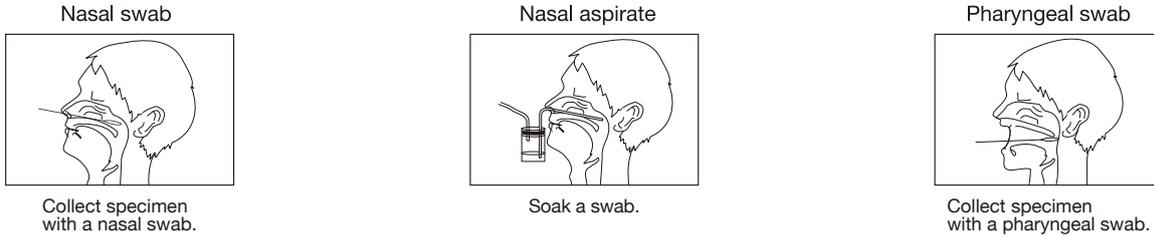


Sample preparation

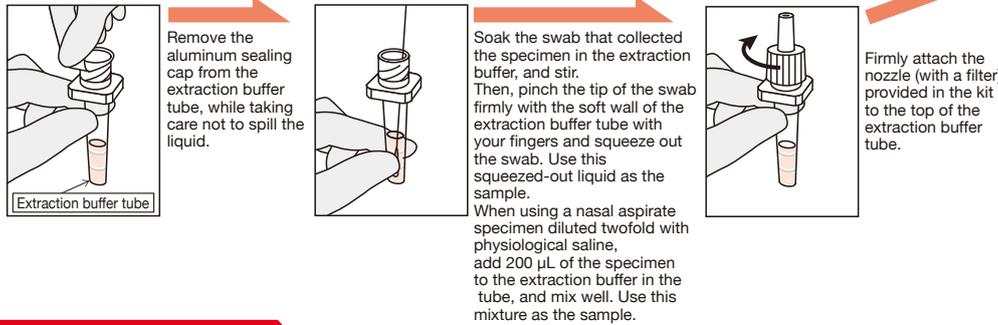

Sample application

Hold the middle of the tube with the fingers and dispense **3** drops of the sample.

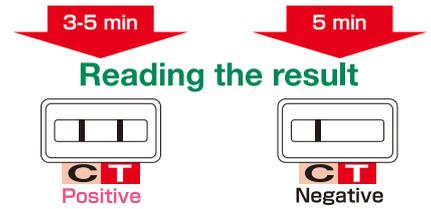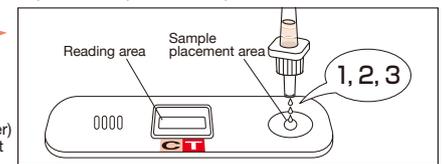

Reference data

Clinical data

The result of the clinical performance evaluation in Japan (Comparison with PCR method)

Kind of sample	Sensitivity (%)	Specificity (%)	Accuracy (%)	Total number
Nasal swab	92.0 (80/87)	100 (104/104)	96.3 (184/191)	191
Nasal aspirate	87.1 (101/116)	100 (179/179)	94.9 (280/295)	295
Pharyngeal swab	91.5 (107/117)	100 (54/54)	94.2 (161/171)	171

Product summary

- **REF** CAHM1670 (20 Tests)
Kit contents: Test Plate \times 20, Extraction Buffer 0.7 mL \times 20, Nozzle \times 20
- **REF** CAHM1671 Test Plate (10 Tests)
Kit content: Test Plate \times 10
- Validity: 27 months
- Storage: Store at 2-30°C
- Reading time: 3-5 minutes